

---

---

**Metallic materials — Vickers  
hardness test —**

**Part 2:  
Verification and calibration of testing  
machines**

*Matériaux métalliques — Essai de dureté Vickers —*

*Partie 2: Vérification et étalonnage des machines d'essai*





**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2018

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva, Switzerland  
Tel. +41 22 749 01 11  
Fax +41 22 749 09 47  
copyright@iso.org  
www.iso.org

Published in Switzerland

# Contents

	Page
<b>Foreword</b> .....	<b>iv</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 General conditions</b> .....	<b>1</b>
<b>5 Direct verification</b> .....	<b>2</b>
5.1 General.....	2
5.2 Calibration of the test force.....	2
5.3 Verification of the indenter.....	3
5.4 Calibration and verification of the diagonal measuring system.....	4
5.5 Verification of the testing cycle.....	5
5.6 Uncertainty of calibration/verification.....	5
<b>6 Indirect verification</b> .....	<b>5</b>
6.1 General.....	5
6.2 Test force and hardness levels.....	5
6.3 Measurement of reference indentation.....	6
6.4 Number of indentations.....	6
6.5 Verification result.....	6
6.6 Repeatability.....	6
6.7 Bias.....	6
6.8 Uncertainty of calibration/verification.....	7
<b>7 Intervals between verifications</b> .....	<b>7</b>
<b>8 Verification report/calibration certificate</b> .....	<b>7</b>
8.1 Vickers testing machine.....	7
8.2 Vickers indenter.....	8
<b>Annex A (informative) Uncertainty of the calibration results of the hardness testing system</b> .....	<b>9</b>
<b>Bibliography</b> .....	<b>18</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 164, *Mechanical testing of metals*, Subcommittee SC 3, *Hardness testing*.

This fourth edition cancels and replaces the third edition (ISO 6507-2:2005), which has been technically revised.

The main changes compared to the previous edition are as follows:

- all references of indentation diagonals, <0,020 mm, have been removed;
- requirements for the calibration and verification of the measuring system have been revised;
- requirements for the maximum permissible error in measuring a reference indentation have been revised;
- recommendations for inspection and monitoring of the indenter have been moved to ISO 6507-1;
- requirements have been added to the test report for reporting the hardness values of reference blocks used;
- Annex A has been revised.

A list of all parts in the ISO 6507 series can be found on the ISO website.

# Metallic materials — Vickers hardness test —

## Part 2: Verification and calibration of testing machines

### 1 Scope

This document specifies a method of verification and calibration of testing machines and diagonal measuring system for determining Vickers hardness in accordance with ISO 6507-1.

A direct method of verification and calibration is specified for the testing machine, indenter and the diagonal length measuring system. An indirect verification method using reference blocks is specified for the overall checking of the machine.

If a testing machine is also to be used for other methods of hardness testing, it shall be verified independently for each method.

This document is also applicable to portable hardness testing machines but not applicable to hardness testing machines based on different measurement principles, e.g. ultrasonic impedance method.

### 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 376, *Metallic materials — Calibration of force-proving instruments used for the verification of uniaxial testing machines*

ISO 6507-1, *Metallic materials — Vickers hardness test — Part 1: Test method*

ISO 6507-3, *Metallic materials — Vickers hardness test — Part 3: Calibration of reference blocks*

### 3 Terms and definitions

No terms and definitions are listed in this document.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <https://www.iso.org/obp>

### 4 General conditions

Before a Vickers hardness testing machine is verified, the machine shall be checked to ensure that it is properly set up in accordance with the manufacturer's instructions.

Especially, it should be checked that:

- a) the plunger holding the indenter is capable of sliding in its guide without any friction or excessive side play;
- b) the indenter-holder is firmly mounted in the plunger;

- c) the test force can be applied and removed without shock, vibration or overshoot and in such a manner that the readings are not influenced;
- d) the diagonal measuring system:
  - 1) if integral with the machine, the change from removing the test force to measuring mode does not influence the readings;
  - 2) the illumination device of the measuring microscope produces uniform lighting of the whole observed field with enough contrast between the indentation and the surrounding surface to determine the boundary clearly;
  - 3) the centre of the indentation is in the centre of the field of view, if necessary.

NOTE The criteria specified in this document for the performance of the testing machine have been developed and refined over a significant period of time. When determining a specific tolerance that the machine needs to meet, the uncertainty associated with the use of measuring equipment and/or reference standards has been incorporated within this tolerance and it would therefore be inappropriate to make any further allowance for this uncertainty by, for example, reducing the tolerance by the measurement uncertainty. This applies to all measurements made when performing a direct or indirect verification of the machine.

## 5 Direct verification

### 5.1 General

5.1.1 Direct verification shall be conducted in accordance with the schedule given in [Clause 7](#).

5.1.2 Direct verification involves:

- a) calibration of the test force;
- b) verification of the indenter;
- c) calibration and verification of the diagonal measuring system;
- d) verification of the testing cycle.

5.1.3 Direct verification should be carried out at a temperature of  $(23 \pm 5)$  °C. If the verification is made outside this temperature range, this shall be stated in the verification report.

5.1.4 The instruments used for verification and calibration shall be traceable to national standards.

### 5.2 Calibration of the test force

5.2.1 Each test force used within the working range of the testing machine shall be measured. Whenever the indenter position affects the applied force, this shall be done at not less than three positions of the plunger uniformly spaced throughout its range of movement during testing.

For testing machines whose test force is shown not to be influenced by the position of the plunger, e.g. closed-loop controlled loading system, the test force can be calibrated in one position.

5.2.2 The test force shall be measured by one of the following methods:

- by means of an elastic proving device in accordance with ISO 376, class 1 or better;
- by balancing against a force, accurate to  $\pm 0,2$  %, applied by means of calibrated masses or another method with the same accuracy.

Evidence should be available to demonstrate that the output of the force-proving device does not vary by more than 0,2 % in the period of 1 s to 30 s following a stepped change in force.

**5.2.3** Three readings shall be taken for each test force,  $F$ , at each position of the plunger. Immediately before each reading is taken, the indenter shall be moved in the same direction as during testing. All readings shall be within the maximum permissible percent relative error,  $\Delta F_{\text{rel}}$ , defined in [Table 1](#).

The percent relative error,  $\Delta F_{\text{rel}}$ , of each measurement of the force,  $F$ , is calculated according to [Formula \(1\)](#):

$$\Delta F_{\text{rel}} = 100 \times \frac{F - F_{\text{RS}}}{F_{\text{RS}}} \quad (1)$$

where

$F$  is the measured test force;

$F_{\text{RS}}$  is the nominal test force.

**Table 1 — Test force tolerances**

Ranges of the nominal test force, $F_{\text{RS}}$	Maximum permissible relative error, $\Delta F_{\text{rel}}$
N	% $F$
$0,009\ 807 \leq F_{\text{RS}} < 0,098\ 07$	$\pm 2,0$
$0,098\ 07 \leq F_{\text{RS}} < 1,961$	$\pm 1,5$
$F_{\text{RS}} \geq 1,961$	$\pm 1,0$

### 5.3 Verification of the indenter

**5.3.1** The four faces of the square-based diamond pyramid shall be polished and free from surface defects.

**5.3.2** The verification of the shape of the indenter can be made by direct measurement or optical measurement. The device used for the verification shall have a maximum expanded uncertainty of 0,07°.

**5.3.3** The measured angles between the opposite faces at the vertex of the diamond pyramid shall be within the range  $136^\circ \pm 0,5^\circ$  (see [Figure 1](#)).

The angles between the opposite faces may also be verified by measuring the angle between the opposite edges. To meet the requirements, the angles between the opposite edges shall be  $148,11^\circ \pm 0,76^\circ$ .

**5.3.4** The angle between the axis of the diamond pyramid and the axis of the indenter-holder (normal to the seating surface) shall be less than 0,5°.

**5.3.5** The four faces should ideally meet at a common point, however, there is usually a line of junction,  $a$ , between opposite faces as shown in [Figure 2](#). The length of the line of junction shall be determined by directly measuring the indenter tip or by measuring the tip impression in an indentation. The maximum permissible length of the line of junction between opposite faces is given in [Table 2](#).

5.3.6 A valid calibration certificate shall exist which confirms the geometrical deviations of the indenter (see 8.2).


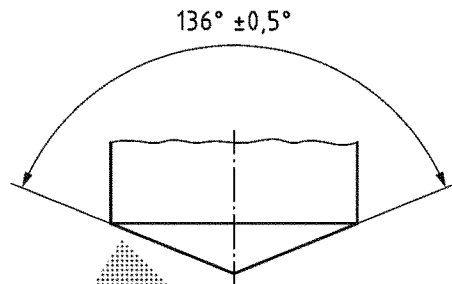


Figure 1 — Angle of the diamond pyramid

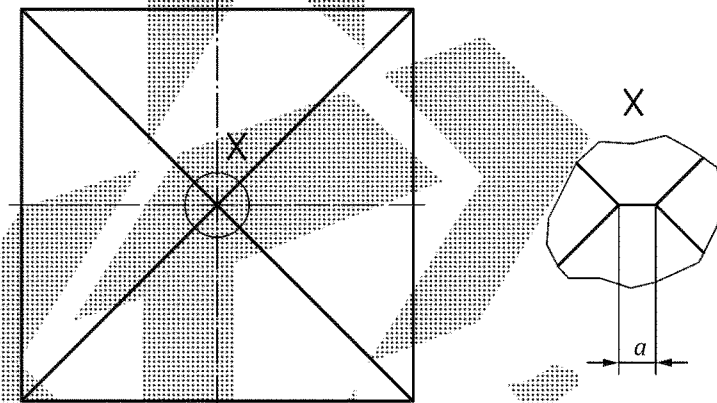

Key

*a* length of line of junction

Figure 2 — Line of junction on the top of the indenter (schematic)

Table 2 — Line of junction tolerance

Ranges of test force, <i>F</i> N	Maximum permissible length of the line of junction, <i>a</i> mm
$0,009\ 807 \leq F < 1,961$	0,000 5
$1,961 \leq F < 49,03$	0,001
$F \geq 49,03$	0,002

## 5.4 Calibration and verification of the diagonal measuring system

5.4.1 The system for measuring the diagonal of the indentation shall be verified at each magnification and for each incorporated line scale to be used. When an individual scale is used in two perpendicular axes, it shall be calibrated in both orientations. Measurements shall be performed using a calibrated stage micrometer. The maximum expanded uncertainty of the distances between the line intervals on the stage micrometer shall be as indicated in Table 3.

5.4.2 Measurements shall be made at a minimum of four evenly spaced intervals, arranged centrally in the field of view, covering each working range. Three measurements shall be made at each of the evenly



spaced intervals. The maximum permissible error of each of the three measurements at each interval shall be as indicated in [Table 3](#).

**Table 3 — Calibration and verification requirements of the measuring system**

Measurement parameters	Calibration and verification requirements
Maximum expanded uncertainty of the distances between the line intervals on the stage micrometer (see <a href="#">5.4.1</a> )	Greater of 0,000 4 mm or 0,2 %
Maximum permissible error of the measurements of the stage micrometer intervals (see <a href="#">5.4.2</a> )	Greater of 0,000 8 mm or 1,0 % of the length measured

## 5.5 Verification of the testing cycle

The testing cycle shall be timed with equipment having a maximum expanded uncertainty of 1 s. The timing values obtained shall fall within the limits set for the testing cycle in ISO 6507-1.

## 5.6 Uncertainty of calibration/verification

Uncertainty of the calibration/verification results shall be determined. An example is given in [Annex A](#).

# 6 Indirect verification

## 6.1 General

**6.1.1** Indirect verification shall be conducted in accordance with the schedule given in [Clause 7](#).

**6.1.2** Indirect verification involves verification of the overall performance of the testing machine by means of reference blocks calibrated in accordance with ISO 6507-3.

**6.1.3** Indirect verification should be carried out at a temperature of  $(23 \pm 5) ^\circ\text{C}$ . If the verification is made outside this temperature range, this shall be reported in the verification report.

**6.1.4** The instruments used for verification and calibration shall be traceable to national standards.

## 6.2 Test force and hardness levels

The testing machine shall be verified by testing reference blocks that have been calibrated in accordance with ISO 6507-3. The blocks shall have been calibrated using the same test forces that the machine will use for future testing. When verifying more than one test force, at least two reference blocks shall be selected from the hardness ranges specified below for each test force that the machine will be verified. The set of blocks needed for verifying the machine for all the test forces shall be chosen so that at least one reference block from each hardness range is used for the verifications. When verifying testing machines using only one test force, three reference blocks shall be used, one from each of the three hardness ranges specified below. The hardness ranges should be chosen, when possible, to replicate the hardness levels most commonly tested when using the specific test forces.

- <250 HV
- 400 HV to 600 HV
- >700 HV

### 6.3 Measurement of reference indentation

One of the reference indentations from the current calibration period on each reference block shall be measured. For each indentation, the difference between the mean measured value and the certified mean diagonal length shall not exceed greater than 0,001 mm or 1,25 % of the reference indentation length. If preferred, this check may instead be made on a similarly-sized indentation in a different reference block with similar hardness.

### 6.4 Number of indentations

On each reference block, five indentations shall be made and measured. The test shall be carried out in accordance with ISO 6507-1. Only the calibrated surfaces of the test blocks are to be used for testing.

### 6.5 Verification result

For each reference block, let  $H_1, H_2, H_3, H_4, H_5$  be the measured hardness arranged in increasing order of magnitude corresponding to the measured diagonals,  $d_1, d_2, d_3, d_4, d_5$ , in decreasing order of magnitude. The mean hardness value,  $\bar{H}$ , is calculated according to Formula (2) and the mean diagonal length,  $\bar{d}$ , is calculated according to Formula (3):

$$\bar{H} = \frac{H_1 + H_2 + H_3 + H_4 + H_5}{5} \quad (2)$$

$$\bar{d} = \frac{d_1 + d_2 + d_3 + d_4 + d_5}{5} \quad (3)$$

### 6.6 Repeatability

The relative repeatability of the testing machine,  $r_{rel}$ , expressed as a percentage of  $\bar{H}$  is calculated according to Formula (4):

$$r_{rel} = 100 \times \frac{H_5 - H_1}{\bar{H}} \quad (4)$$

The repeatability of the testing machine is satisfactory if  $(d_1 - d_5) \leq 0,001$  mm. If  $(d_1 - d_5) > 0,001$  mm, the testing machine is satisfactory if  $r_{rel}$  is less than or equal to the percentages indicated in Table 4.

**Table 4 — Maximum permissible relative repeatability**

Vickers hardness of the reference block	Maximum permissible relative HV repeatability of the testing machine, $r_{rel}$ %HV		
	HV 5 to HV 100	HV 0,2 to < HV 5	< HV 0,2
HV ≤250	6,0	12,0	18,0
HV >250	4,0	8,0	12,0

NOTE Lower hardness materials often exhibit higher values of repeatability than those for higher hardness materials.

### 6.7 Bias

The bias,  $b$ , of the testing machine under the particular verification conditions is calculated according to Formula (5):

$$b = \bar{H} - H_{CRM} \quad (5)$$

where  $H_{CRM}$  is the certified hardness of the reference block used.

The percent bias,  $b_{rel}$ , is calculated according to Formula (6):

$$b_{rel} = 100 \times \frac{\bar{H} - H_{CRM}}{H_{CRM}} \quad (6)$$

The maximum positive or negative bias of the testing machine, expressed as a percentage of the specified hardness of the reference block, shall not exceed the values given in Table 5.

**Table 5 — Maximum permissible percent HV bias**

Mean diagonal length, $\bar{d}$ mm	Maximum permissible percent HV bias, $b_{rel}$ , of the testing machine $\pm$ %HV
$0,02 \leq \bar{d} < 0,14$	$0,21/\bar{d} + 1,5$
$0,14 \leq \bar{d} \leq 1,4$	3

## 6.8 Uncertainty of calibration/verification

Uncertainty of the calibration results shall be determined. An example is given in Annex A.

## 7 Intervals between verifications

Direct verifications shall be performed according to the schedule given in Table 6. It is recommended that direct verifications be performed every 12 months.

Indirect verification shall be performed at least once every 12 months and after a direct verification has been performed.

**Table 6 — Direct verifications of hardness testing machines**

Requirements of verification	Force	Diagonal measuring system	Test cycle	Indenter <sup>a</sup>
Before setting to work first time	x	x	x	x
After dismantling and reassembling, if force, diagonal measuring system or test cycle are affected.	x	x	x	
Failure of indirect verification <sup>b</sup>	x	x	x	
Indirect verification > 13 months ago	x	x	x	

<sup>a</sup> In addition, it is recommended that the indenter be directly verified after 2 years of use.

<sup>b</sup> Direct verification of these parameters may be carried out sequentially (until the machine passes indirect verification) and is not required if it can be demonstrated, for example, by tests with a reference indenter, that the indenter was the cause of the failure.

## 8 Verification report/calibration certificate

### 8.1 Vickers testing machine

The verification report/calibration certificate shall include the following information:

- a reference to this document, i.e. ISO 6507-2;
- the method of verification (direct and/or indirect);
- identification data of the hardness testing machine;

- d) means of verification (reference blocks, elastic proving devices, etc.);
- e) test force(s) verified;
- f) hardness values of reference blocks used;
- g) the verification temperature, if outside the range specified in 5.1.4;
- h) all results obtained;
- i) the date of verification and reference to the verification institution;
- j) the uncertainty of the verification result.

## 8.2 Vickers indenter

The verification report/calibration certificate shall include the following information:

- a) a reference to this document, i.e. ISO 6507-2;
- b) the indenter serial number;
- c) all results obtained;
- d) the date of verification and reference to the verification institution;
- e) the uncertainty of the verification result.

## Annex A (informative)

### Uncertainty of the calibration results of the hardness testing system

#### A.1 General

Measurement uncertainty analysis is a useful tool to help determine sources of error and to understand differences between measured values. This annex gives guidance on uncertainty estimation but the values derived are for information only unless specifically instructed otherwise by the customer. The criteria specified in this document for the performance of the testing machine have been developed and refined over a significant period of time. When determining a specific tolerance that the machine needs to meet, the uncertainty associated with the use of measuring equipment and/or reference standards has been incorporated within this tolerance and it would therefore be inappropriate to make any further allowance for this uncertainty by, for example, reducing the tolerance by the measurement uncertainty. This applies to all measurements made when performing a direct or indirect verification of the machine. In each case, it is simply the measured value resulting from the use of the specified measuring equipment and/or reference standards that is used to assess whether or not the machine complies with this document. However, there may be special circumstances where reducing the tolerance by the measurement uncertainty is appropriate. This should only be done by agreement of the parties involved.

The metrological chain necessary to define and disseminate hardness scales is discussed in ISO 6507-1.

#### A.2 Direct verification of the hardness testing machine

##### A.2.1 Calibration of the test force

The combined relative standard uncertainty of the test force calibration is calculated according to Formula (A.1):

$$u_F = \sqrt{u_{FRS}^2 + u_{FHTM}^2} \quad (\text{A.1})$$

where

$u_{FRS}$  is the relative uncertainty of measurement of the force transducer (from the calibration certificate);

$u_{FHTM}$  is the relative standard uncertainty of the test force generated by the hardness testing machine.

The uncertainty of measurement of the reference instrument, force transducer, is indicated in the corresponding calibration certificate. The influence quantities, like

- temperature dependence,
- long-term stability, and
- interpolation deviation,

should be considered for critical applications. Depending on the design of the force transducer, the rotational position of the transducer related to the indenter axis of the hardness testing machine should be considered.

EXAMPLE

Using the results shown in [Table A.1](#) and the following information:

- uncertainty of measurement of the force transducer (from calibration certificate):  $U_{FRS} = 0,12\%$  ( $k = 2$ ), and
- calibration value of the force transducer:  $F_{RS} = 294,2\text{ N}$ ,

the combined relative standard uncertainty of the test force calibration,  $u_F$ , is calculated according to [Formula \(A.1\)](#) and as shown in [Table A.2](#).

In [Table A.1](#), the relative deviation is calculated according to [Formula \(A.2\)](#):

$$\Delta F_{rel,i,j} = \frac{F_{i,j} - F_{RS}}{F_{RS}} \tag{A.2}$$

where  $F_{ij}$  is the test-force measurement value in the  $i$ -th height position of the  $j$ -th measurement series.

The relative standard uncertainty is calculated according to [Formula \(A.3\)](#):

$$u_{FHTM,i} = \frac{s_{F_i}}{F_i} \times \frac{t}{\sqrt{n}} \quad (n = 3, t = 1,32) \tag{A.3}$$

where  $s_{F_i}$  is the standard deviation of the test-force indication values in the  $i$ -th height position.

**Table A.1 — Results of the test force calibration**

Number of height position ( $i$ ) for test force calibration	Series 1		Series 2		Series 3		Mean value	Standard deviation	Relative standard uncertainty
	Value	Relative deviation	Value	Relative deviation	Value	Relative deviation			
	$F_{i,1}$	$\Delta F_{rel,i,1}$	$F_{i,2}$	$\Delta F_{rel,i,2}$	$F_{i,3}$	$\Delta F_{rel,i,3}$			
N	%	N	%	N	%	N	N		
1	294,7	0,170	294,9	0,238	294,5	0,102	294,7	0,200	$0,52 \times 10^{-3}$
2	293,9	-0,102	294,5	0,102	294,6	0,136	294,3	0,379	$0,98 \times 10^{-3}$
3	293,1	-0,374	294,0	-0,068	293,7	-0,170	293,6	0,458	$1,19 \times 10^{-3}$

In [Table A.2](#), the uncertainty of the measurement of the test force is determined using the maximum value of relative standard uncertainty,  $u_{FHTM,i}$ , from [Table A.1](#) (in this case,  $u_{FHTM,3}$ ).

Table A.2 — Calculation of the uncertainty of measurement of the test force

Quantity	Estimated value	Relative limit values	Distribution type	Symbol	Relative standard uncertainty	Sensitivity coefficient	Relative uncertainty contribution
$X_p$	$x_p$	$a_p$			$u(x_p)$	$c_p$	$u_p(F)$
Force transducer indication	294,2 N	±0,12 %	Normal	$u_{FRS}$	$0,6 \times 10^{-3}$	1	$0,6 \times 10^{-3}$ N
Accuracy of generated force	0 N	±1 %	Normal	$u_{FHTM}$	$1,19 \times 10^{-3}$	1	$1,19 \times 10^{-3}$ N
Relative combined standard uncertainty, $u_F$ , %							0,133
Relative expanded uncertainty of measurement, $U_F$ ( $k = 2$ ), %							0,266

In Table A.3, the maximum relative deviation of the test force including the uncertainty of measurement of the reference instrument is calculated according to Formula (A.4) using the maximum absolute value of  $\Delta F_{rel,i,j}$  from Table A.1 (in this case,  $\Delta F_{rel,3,1}$ ).

$$\Delta F_{\max} = |\Delta F_{rel,i,j}| + U_F \quad (A.4)$$

Table A.3 — Calculation of the maximum relative deviation of the test force including the uncertainty of measurement of the reference instrument

Maximum relative deviation of test force $\Delta F_{rel,3,1}$	Expanded relative measurement uncertainty of test force $U_F$	Max. relative deviation of test force including measurement uncertainty of reference instrument $\Delta F_{\max}$
-0,374 %	0,266 %	0,640 %

$\Delta F_{\max}$  is calculated according to Formula (A.5):

$$\Delta F_{\max} = |\Delta F_{rel}| + U_F \quad (A.5)$$

The result of the example means that the deviation of the test force, including the uncertainty of measurement of the reference instrument specified in 5.4 amounting to ±1,0 % is complied with.

## A.2.2 Calibration of the diagonal measuring system

The combined relative standard uncertainty of the reference instrument for the diagonal measuring system is calculated according to Formula (A.6):

$$u_L = \sqrt{u_{LRS}^2 + 2 \times u_{ms}^2 + u_{LHTM}^2} \quad (A.6)$$

where

$u_{LRS}$  is the relative uncertainty of measurement of the stage micrometer (reference standard) from the calibration certificate for  $k = 1$ ;

$u_{ms}$  is the relative uncertainty of measurement due to the resolution of the diagonal measuring system;

$u_{LHTM}$  is the relative standard uncertainty of measurement of the diagonal measuring system of the hardness testing machine.

Regarding  $u_{ms}$ , both the resolution of the length measurement indicating the instrument and the optical resolution of the measuring microscope shall be considered. In most cases, the overall resolution of the measurement system should be included twice in the calculation of  $u_L$  due to resolving the positions of both the zero and indicator lines of the stage micrometer.

The uncertainty of measurement of the reference instrument for the diagonal measuring system, the stage micrometer, is indicated in the corresponding calibration certificate. The influence quantities, for example,

- temperature dependence,
- long-term stability, and
- interpolation deviation,

do not exert an essential influence on the uncertainty of measurement of the stage micrometer.

EXAMPLE

For this example, five indication intervals are measured (0,05 mm, 0,10 mm, 0,20 mm, 0,30 mm and 0,40 mm).

Using the results as shown in Table A.4 and the following information:

- uncertainty of measurement of the stage micrometer:  $U_{LRS} = 0,000\ 1\ \text{mm}$  ( $k = 2$ )
- optical resolution of the microscope objective:  $\delta_{OR} = 0,000\ 34\ \text{mm}$

NOTE  $\delta_{OR} = \lambda / (2 \times \text{NA})$

where

$\lambda$  is the wave length of light in  $\mu\text{m}$  (approx.  $0,55\ \mu\text{m}$  for green light);

NA is the numerical aperture of the objective.

EXAMPLE For a  $100\times$  objective with an NA of 0,8 using green light,  $\delta_{OR} = 0,55\ \mu\text{m} / (2 \times 0,8) = 0,34\ \mu\text{m}$ .

The above optical resolution formula is valid for lighting inclined at large angles.

- resolution of the display indicator of the measuring system:  $\delta_R = 0,000\ 1\ \text{mm}$ ;
- the resolution of the diagonal measuring system is calculated according to Formula (A.7):

$$\delta_{ms} = \sqrt{\delta_{OR}^2 + \delta_{IR}^2} = 0,000\ 35\ \text{mm} \tag{A.7}$$

the combined relative standard uncertainty of the reference instrument for the diagonal measuring system,  $u_L$ , is calculated according to Formula (A.6) and as shown in Table A.5.

In Table A.4, the relative deviation  $\Delta L_{rel,i,j}$  for the  $i$ -th indication interval of the  $j$ -th measurement series of the stage micrometer is calculated according to Formula (A.8):

$$\Delta L_{rel,i,j} = \frac{L_{i,j} - L_{RS,i}}{L_{RS,i}} \times 100 \tag{A.8}$$

where

$L_{RS,i}$  is the  $i$ -th indication interval value of the stage micrometer;

$L_{i,j}$  is the length measurement value for the  $i$ -th indication interval of the  $j$ -th measurement series of the stage micrometer.



Table A.4 — Results of the calibration of the diagonal measuring system

Number of indication interval	Indication interval value ( <i>i</i> ) of the stage micrometer	Series 1		Series 2		Series 3		Mean value	Standard deviation mm
		Value	Relative deviation	Value	Relative deviation	Value	Relative deviation		
<i>i</i>	$L_{RS,i}$ mm	$L_{i,1}$ mm	$\Delta L_{rel,i,1}$ %	$L_{i,2}$ mm	$\Delta L_{rel,i,2}$ %	$L_{i,3}$ mm	$\Delta L_{rel,i,3}$ %	$\bar{L}_i$ mm	$s_{L_i}$
1	0,05	0,050 0	0,000	0,050 0	0,000	0,050 1	0,200	0,050 0	0,000 058
2	0,10	0,100 2	0,200	0,100 0	0,000	0,100 1	0,100	0,100 1	0,000 100
3	0,20	0,200 1	0,050	0,199 9	-0,050	0,200 1	0,050	0,200 0	0,000 115
4	0,30	0,299 7	0,100	0,300 1	0,033	0,300 1	0,033	0,300 0	0,000 231
5	0,40	0,400 2	0,050	0,400 1	0,025	0,400 3	0,075	0,400 2	0,000 100

The standard uncertainty of measurement of the diagonal measuring system,  $u_L$ , is calculated in accordance with Formula (A.6). The contributions to the calculation are given in Table A.5 and calculated as follows.

The relative standard uncertainty of measurement of the stage micrometer for the *i*-th indication interval is calculated according to Formula (A.9):

$$u_{LRS,i} = \frac{U_{LRS}/2}{L_{RS,i}} \quad (\text{A.9})$$

The relative standard uncertainty due to the resolution of the diagonal measuring system for the *i*-th indication interval is calculated according to Formula (A.10):

$$u_{ms,i} = \frac{\delta_{ms}/2\sqrt{3}}{L_{RS,i}} \quad (\text{A.10})$$

The relative standard uncertainty of the measurements of the *i*-th indication interval is calculated according to Formula (A.11):

$$u_{LHTM,i} = \frac{s_{L_i}}{L_i} \times \frac{t}{\sqrt{n}} \quad (n=3, t=1,32) \quad (\text{A.11})$$

where

$s_{L_i}$  is the standard deviation of the length measurement values for the *i*-th indication interval of the stage micrometer;

$\bar{L}_i$  is the mean length measurement value for the *i*-th indication interval of the stage micrometer.

Table A.5 — Calculation of the uncertainty of measurement of the diagonal measuring system

Quantity $X_p$	Distribu- tion type	Estimat- ed value $x_p$	Sym- bol	Formula: Relative standard uncertainty $u(x_p)$	Sens. coeff. $c_p$	Relative uncertainty contribution, $u_p(L)$				
						$L_{RS,1}$ (0,05 mm)	$L_{RS,2}$ (0,10 mm)	$L_{RS,3}$ (0,20 mm)	$L_{RS,4}$ (0,30 mm)	$L_{RS,5}$ (0,40 mm)
Stage microm- eter	Normal	$L_{RS,i}$	$u_{LRS}$	$u_{LRS,i} = \frac{u_{LRS}}{L_{RS,i}}$	1	$1,00 \times 10^{-3}$	$0,50 \times 10^{-3}$	$0,25 \times 10^{-3}$	$0,17 \times 10^{-3}$	$0,13 \times 10^{-3}$
Resolu- tion of the diago- nal meas- uring system (include twice)	Rectan- gular	0,000 35 mm	$u_{ms}$	$u_{ms,i} = \frac{\delta_{ms}}{L_{RS,i} \cdot 2\sqrt{3}}$	1	$2,28 \times 10^{-3}$	$1,14 \times 10^{-3}$	$0,57 \times 10^{-3}$	$0,38 \times 10^{-3}$	$0,28 \times 10^{-3}$
Accura- cy of the diago- nal meas- uring system	Normal	$L_{RS,i}$	$u_{LITM}$	$u_{LITM,i} = \frac{s_{Li} \times t}{L_i \sqrt{n}}$ ( $n = 3; t = 1,32$ )	1	$0,88 \times 10^{-3}$	$0,76 \times 10^{-3}$	$0,44 \times 10^{-3}$	$0,59 \times 10^{-3}$	$0,19 \times 10^{-3}$
Relative combined uncertainty of measurement, $u_{p,i}$ , %						0,349	0,185	0,095	0,081	0,046
Relative expanded uncertainty of measurement, $U_{L,i}$ ( $k = 2$ ), %						0,697	0,370	0,190	0,163	0,093

In Table A.6, the maximum relative deviation of the diagonal measuring system including the uncertainty of measurement of the length reference instrument,  $\Delta L_{max,i}$ , for the  $i$ -th indication interval of the stage micrometer is calculated according to Formula (A.12):

$$\Delta L_{max,i} = \max|\Delta L_{rel,i}| + U_{L,i} \tag{A.12}$$

where  $\max|\Delta L_{rel,i}|$  is the maximum absolute value of the relative deviations  $\Delta L_{rel,i,j}$  for the  $i$ -th indication interval of the stage micrometer from Table A.4.

Table A.6 — Calculation of the maximum relative deviation of the diagonal measuring system including the uncertainty of measurement of the length reference instrument

Number of indication interval $i$	Indication interval value ( $i$ ) of the stage micrometer $L_{RS,i}$	Maximum relative deviation of the diagonal measuring system $\max \Delta L_{rel,i} $	Expanded relative uncertainty of measure- ment $U_{L,i}$	Max. relative deviation of diagonal measuring system including uncertainty of length reference instrument $\Delta L_{max,i}$	Maximum permissible relative deviation specified in 5.4
1	0,05 mm	0,20 %	0,70 %	0,90 %	1,2 %
2	0,10 mm	0,20 %	0,37 %	0,57 %	1,0 %
3	0,20 mm	0,05 %	0,19 %	0,24 %	1,0 %
4	0,30 mm	0,10 %	0,16 %	0,26 %	1,0 %
5	0,40 mm	0,07 %	0,09 %	0,17 %	1,0 %

The result of the example means that the deviation of the diagonal measuring system, including the uncertainty of measurement of the length reference instrument specified in 5.4 is complied with for each of the indication intervals of the stage micrometer.

### A.2.3 Verification of the indenter

The indenter, consisting of indenter tip and holder, cannot be verified, respectively calibrated in-site (see 5.3).

### A.2.4 Verification of the test cycle

While measuring with a usual time-measuring system (stopwatch), the uncertainty of measurement can be indicated as 0,1 s. Therefore, an estimation of the uncertainty of measurement is not necessary.

## A.3 Indirect verification of the hardness testing machine

By indirect verification with hardness reference blocks, the overall function of the hardness testing machine is checked and the repeatability, as well as the deviation of the hardness testing machine from the real hardness value, are determined.

NOTE In this annex, the index "certified reference material" (CRM) means, according to the definitions of the hardness testing standards, "hardness reference block".

The uncertainty of measurement of the indirect verification of the hardness testing machine is calculated according to Formula (A.13):

$$u_{\text{HTM}} = \sqrt{u_{\text{CRM}}^2 + u_{\text{CRM-D}}^2 + u_{\text{H}}^2 + 2 \times u_{\text{ms}}^2} \quad (\text{A.13})$$

where

- $u_{\text{CRM}}$  is the calibration uncertainty of the hardness reference block according to the calibration certificate for  $k = 1$ ;
- $u_{\text{CRM-D}}$  is the hardness change of the hardness reference block since its last calibration due to drift (negligible for use of the hardness reference block complying with the document);
- $u_{\text{HCRM}}$  is the standard uncertainty of the hardness testing machine when measuring the CRM;
- $u_{\text{ms}}$  is the uncertainty due to the resolution of the diagonal measuring system of the hardness testing machine. Both the resolution of the length measurement indicating instrument and the optical resolution of the measuring microscope shall be considered. In most cases, the overall resolution of the measurement system should be included twice in the calculation of  $u_{\text{HTM}}$  due to resolving the positions of both ends of the long diagonal independently.

#### EXAMPLE

Using results as shown in Table A.7 and the following information:

- hardness of the hardness reference block:  $H_{\text{CRM}} = 400,0 \text{ HV } 30$
- uncertainty of measurement of the hardness reference block:  $U_{\text{CRM}} = 5,0 \text{ HV } 30, k = 2$
- resolution of the diagonal measuring system of the hardness testing machine:  
 $\delta_{\text{ms}} = 0,000 \text{ 35 mm}$   
 calculated according to Formula (A.14):

$$\delta_{ms} = \sqrt{\delta_{OR}^2 + \delta_{IR}^2} \tag{A.14}$$

where

$\delta_{OR}$  is the optical resolution of the microscope objective (0,000 34 mm) (see the example in A.2.2);

$\delta_{IR}$  is the resolution of the display indicator of the measuring system (0,000 1 mm);

$u_{ms}$  is the standard uncertainty of measurement due to the resolution of the diagonal measuring system (rectangular distribution),  $\left( \frac{0,000\ 35}{2\sqrt{3}} = 0,000\ 102\ \text{mm} \right)$ ,

the uncertainty of measurement of the indirect verification of the hardness testing machine,  $u_{HTM}$ , is calculated according to Formula (A.13) and as shown in Table A.8.

**Table A.7 — Results of the indirect verification**

No.	Measured indentation diagonal $d$ , mm	Calculated hardness value $H$ , HV30 <sup>a</sup>
1	0,371 6 <sub>min</sub>	402,9 <sub>max</sub>
2	0,372 4	401,1
3	0,372 8 <sub>max</sub>	400,3 <sub>min</sub>
4	0,371 9	402,2
5	0,372 2	401,5
Mean value, $\bar{H}$	0,372 2	401,6
Standard deviation, $s_H$		0,99

<sup>a</sup> HV: Vickers hardness.

The bias of the hardness testing system is determined according to Formula (A.15):

$$b = \bar{H} - H_{CRM} \tag{A.15}$$

$$b = 401,6 - 400,0 = 1,6\ \text{HV}\ 30$$

The standard uncertainty of the hardness testing machine when measuring the CRM is calculated according to Formula (A.16):

$$u_{HCRM} = \frac{t - s_H}{\sqrt{n}} \tag{A.16}$$

For  $t = 1,14$ ,  $n = 5$  and  $s_H = 0,99\ \text{HV}\ 30$ ,

$$u_{HCRM} = 0,51\ \text{HV}\ 30$$

#### A.4 Budget of uncertainty of measurement

The contribution of each element to the combined uncertainty of measurement is given in Table A.8 and the maximum deviation of the hardness testing machine including the uncertainty of measurement is shown in Table A.9.

Table A.8 — Budget of uncertainty of measurement

Quantity	Estimated value	Standard uncertainty of measurement	Distribution type	Sensitivity coefficient	Uncertainty contribution
$X_p$	$x_p$	$u(x_p)$		$c_p$	$u_p(H)$ HV 30
$u_{CRM}$	400 HV <sup>b</sup>	2,50 HV 30	Normal	1,0	2,50
$u_{HCRM}$	0 HV	0,51 HV 30	Normal	1,0	0,51
$u_{ms}$	0 mm	0,000 102 mm	Rectangular	-2 145,1 <sup>a</sup>	-0,22
$u_{CRM-D}$	0 HV	0 HV 30	Triangular	1,0	0
Combined uncertainty of measurement, $u_{HTM}$					2,57
Expanded uncertainty of measurement, $U_{HTM}$ ( $k = 2$ )					5,14

<sup>a</sup> The sensitivity coefficient follows from  $c = \partial H / \partial d = -2(H/d)$  for  $H = 400$  HV 30 and  $d \approx 0,372 9$  mm.

The maximum deviation of the testing machine including the uncertainty of measurement is calculated according to Formula (A.17) as shown in Table A.9.

$$\Delta H_{HTMmax} = U_{HTM} + |b| = 5,1 \text{ HV 30} + 1,6 \text{ HV 30} = 6,8 \text{ HV 30} \quad (\text{A.17})$$

Table A.9 — Maximum deviation of the hardness testing machine including the uncertainty of measurement

Measured mean hardness on the hardness testing machine	Expanded uncertainty of measurement	Deviation of the testing machine when calibrating with the reference block	Maximum deviation of the testing machine including uncertainty of measurement
$\bar{H}$	$U_{HTM}$	$ b $	$\Delta H_{HTMmax}$
401,6 HV 30	5,14 HV 30	1,62 HV 30	6,76 HV 30

The relative deviation of the testing machine including uncertainty of measurement is calculated according to Formula (A.18):

$$\frac{\Delta H_{HTMmax}}{\bar{H}} = \frac{6,8}{401,6} = 1,7 \% \quad (\text{A.18})$$

## Bibliography

- [1] SAWLA A. *Uncertainty of measurement in the verification and calibration of the force measuring systems of testing machines*, Proceedings of the Asia-Pacific symposium on measurement of force, mass and torque (APMF), Tsukuba, Japan, Novembre 2000
- [2] WEHRSTEDT A., & PATKOVSKY I. *News in the field of standardization about verification and calibration of materials testing machines*, May 2001, EMPA Academy 2001
- [3] GABAUER W. Manual codes of practice for the determination of uncertainties in mechanical tests on metallic materials, The estimation of uncertainties in hardness measurements, Project No. SMT4-CT97-2165, UNCERT COP 14, 2000
- [4] POLZIN T., & SCHWENK D. Method for Uncertainty Determination of Hardness Testing; PC File for Determination, *Materialprüfung* 44 ( 2002) 3, pp. 64–71

